


Viability of Eye-tracking Glasses for Beamforming Hearing-Aids

Emily Steiner

Department of Electrical Engineering, Stanford University

Motivation


- Current assistive hearing technology is limited in aiding selective attention in complex auditory 'cocktail party' environments
- Beamforming leverages time delay information between sensors in a phased array to spatially direct sound amplification
- We want to evaluate the **relative benefit of using eye-tracking versus head-movement** as a steering technique for the hardware limitations of a beamforming pair of glasses

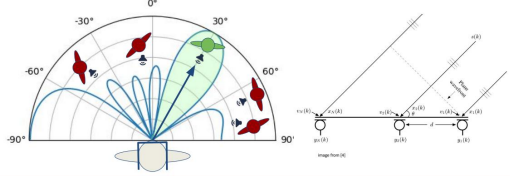


Simulation & Implementation

Evaluation of Minimum Variance Distortionless Response (MVDR) beamforming (adaptive) in simulations of predicted use cases — evaluation of ability to resolve sources at small angles

Broadband Beamforming [4][5]

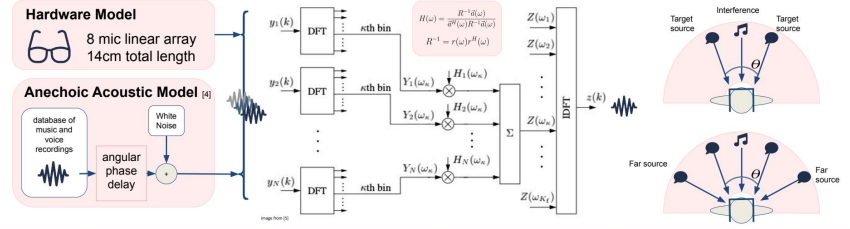

Scenarios



Related Work

Nuance Hearing [1]

- Collar microphone array
- **Practical utility of a head-mounted gaze-directed beamforming system [2]**


A visually guided beamformer to aid listening in complex acoustic environments [3]

- User study evaluating non-adaptive beamforming
- 4x4 microphone grid, three beam selection to maintain binaural information

References

- [1] Y. H. et al., "Directional hearing aid," U.S. Patent 0 567 888B2, Feb. 18, 2020.
- [2] F. Culling, et al., "Practical utility of a head-mounted gaze-directed beamforming system," The Journal of the Acoustical Society of America, 2023
- [3] T. R. Jennings and G. Kidd, "A visually guided beamformer to aid listening in complex acoustic environments," in Proceedings of Meetings on Acoustics, 2018.
- [4] J. Benesty, J. Chen, and Y. Huang, Microphone array signal processing. Springer Science & Business Media, 2008, vol. 1.
- [5] H. Van Trees, Optimum Array Processing. John Wiley Sons, Ltd, 2002.

Experimental Results

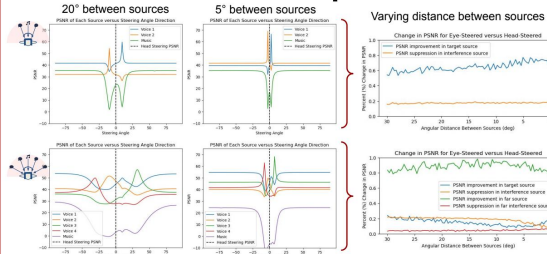

Discussion:

- High variation in measurements (dependant on audio clips used)
- Number of sources far outweighs distance between sources
- Qualitative output does not always match PSNR improvement

Limitations: simulation model, real-time time windowing, assumption that eye-tracking represents ground truth, far-field point sources, number of audio clips

- Future Work**
- Simulation (image-source model, time-windowing) & metrics (directivity index, word error rate)
 - Prototype and user study for evaluation of ease and convenience
 - Investigation into NN/probabilistic attention models, SSS