

# BCA™ Protein Assay Kit

23225 23227

1296.3

Number	Description
23225	BCA™ Protein Assay Kit, sufficient reagents for 500 test tube or 5,000 microplate assays
23227	BCA™ Protein Assay Kit, sufficient reagents for 250 test tube or 2,500 microplate assays

### Kit Contents:

**BCA™ Reagent A**, 1,000 ml (in Product No. 23225) or 500 ml (in Product No. 23227), containing sodium carbonate, sodium bicarbonate, bicinchoninic acid and sodium tartrate in 0.1 M sodium hydroxide

**BCA™ Reagent B**, 25 ml, containing 4% cupric sulfate

**Albumin Standard Ampules, 2 mg/ml**, 10 x 1 ml ampules, containing bovine serum albumin (BSA) at 2.0 mg/ml in 0.9% saline and 0.05% sodium azide

**Storage:** Upon receipt store at room temperature. Product shipped at ambient temperature.

**Note:** If either Reagent A or Reagent B precipitates upon shipping in cold weather or during long-term storage, dissolve precipitates by gently warming and stirring solution. Discard any kit reagent that shows discoloration or evidence of microbial contamination.

## Table of Contents

Introduction.....	1
Preparation of Standards and Working Reagent (required for both assay procedures).....	2
Test Tube Procedure (Sample to WR ratio = 1:20) .....	3
Microplate Procedure (Sample to WR ratio = 1:8).....	3
Troubleshooting.....	4
Related Pierce Products .....	5
Additional Information .....	5
Cited References.....	6
Product References .....	6

## Introduction

The BCA™ Protein Assay is a detergent-compatible formulation based on bicinchoninic acid (BCA) for the colorimetric detection and quantitation of total protein. This method combines the well-known reduction of  $\text{Cu}^{+2}$  to  $\text{Cu}^{+1}$  by protein in an alkaline medium (the biuret reaction) with the highly sensitive and selective colorimetric detection of the cuprous cation ( $\text{Cu}^{+1}$ ) using a unique reagent containing bicinchoninic acid.<sup>1</sup> The purple-colored reaction product of this assay is formed by the chelation of two molecules of BCA with one cuprous ion. This water-soluble complex exhibits a strong absorbance at 562 nm that is nearly linear with increasing protein concentrations over a broad working range (20-2,000  $\mu\text{g/ml}$ ). The BCA™ method is not a true end-point method; that is, the final color continues to develop. However, following incubation, the rate of continued color development is sufficiently slow to allow large numbers of samples to be assayed together.

The macromolecular structure of protein, the number of peptide bonds and the presence of four particular amino acids (cysteine, cystine, tryptophan and tyrosine) are reported to be responsible for color formation with BCA.<sup>2</sup> Studies with di-, tri- and tetrapeptides suggest that the extent of color formation caused by more than the mere sum of individual color-producing functional groups.<sup>2</sup> Accordingly, protein concentrations generally are determined and reported with reference to standards of a common protein such as bovine serum albumin (BSA). A series of dilutions of known concentration are

**Warranty:** Pierce products are warranted to meet stated product specifications and to conform to label descriptions when used and stored properly. Unless otherwise stated, this warranty is limited to one year from date of sale for products used, handled and stored according to Pierce instructions. Pierce's sole liability for the product is limited to replacement of the product or refund of the purchase price. Pierce products are supplied for laboratory or manufacturing applications only. They are not intended for medicinal, diagnostic or therapeutic use. Pierce products may not be resold, modified for resale or used to manufacture commercial products without prior written approval from Pierce Biotechnology. Pierce strives for 100% customer satisfaction. If you are not satisfied with the performance of a Pierce product, please contact Pierce or your local distributor.

prepared from the protein and assayed alongside the unknown(s) before the concentration of each unknown is determined based on the standard curve. If precise quantitation of an unknown protein is required, it is advisable to select a protein standard that is similar in quality to the unknown; for example, a bovine gamma globulin (BGG) standard (see Related Pierce Products) may be used when assaying immunoglobulin samples.

Two assay procedures are presented. Of these, the Test Tube Procedure requires a larger volume (0.1 ml) of protein sample; however, because it uses a sample to working reagent ratio of 1:20 (v/v), the effect of interfering substances is minimized. The Microplate Procedure affords the sample handling ease of a microplate and requires a smaller volume (10-25  $\mu$ l) of protein sample; however, because the sample to working reagent ratio is 1:8 (v/v), it offers less flexibility in overcoming interfering substance concentrations and obtaining low levels of detection.

## Preparation of Standards and Working Reagent (required for both assay procedures)

### A. Preparation of Diluted Albumin (BSA) Standards

Use Table 1 as a guide to prepare a set of protein standards. Dilute the contents of one Albumin Standard (BSA) ampule into several clean vials, preferably using the same diluent as the sample(s). Each 1 ml ampule of 2.0 mg/ml Albumin Standard is sufficient to prepare a set of diluted standards for either working range suggested in Table 1. There will be sufficient volume for three replications of each diluted standard.

**Table 1.** Preparation of Diluted Albumin (BSA) Standards

Dilution Scheme for Standard Test Tube Protocol and Microplate Procedure (Working Range = 20–2,000 g/ml)			
<u>Vial</u>	<u>Volume of Diluent</u>	<u>Volume and Source of BSA</u>	<u>Final BSA Concentration</u>
A	0	300 $\mu$ l of Stock	2,000 g/ml
B	125 $\mu$ l	375 $\mu$ l of Stock	1,500 g/ml
C	325 $\mu$ l	325 $\mu$ l of Stock	1,000 g/ml
D	175 $\mu$ l	175 $\mu$ l of vial B dilution	750 g/ml
E	325 $\mu$ l	325 $\mu$ l of vial C dilution	500 g/ml
F	325 $\mu$ l	325 $\mu$ l of vial E dilution	250 g/ml
G	325 $\mu$ l	325 $\mu$ l of vial F dilution	125 g/ml
H	400 $\mu$ l	100 $\mu$ l of vial G dilution	25 g/ml
I	400 $\mu$ l	0	0 g/ml = Blank
Dilution Scheme for Enhanced Test Tube Protocol (Working Range = 5–250 g/ml)			
<u>Vial</u>	<u>Volume of Diluent</u>	<u>Volume and Source of BSA</u>	<u>Final BSA Concentration</u>
A	700 $\mu$ l	100 $\mu$ l of Stock	250 g/ml
B	400 $\mu$ l	400 $\mu$ l of vial A dilution	125 g/ml
C	450 $\mu$ l	300 $\mu$ l of vial B dilution	50 g/ml
D	400 $\mu$ l	400 $\mu$ l of vial C dilution	25 g/ml
E	400 $\mu$ l	100 $\mu$ l of vial D dilution	5 g/ml
F	400 $\mu$ l	0	0 g/ml = Blank

### B. Preparation of the BCA™ Working Reagent (WR)

- Use the following formula to determine the total volume of WR required:

$$(\# \text{ standards} + \# \text{ unknowns}) \times (\# \text{ replicates}) \times (\text{volume of WR per sample}) = \text{total volume WR required}$$

Example: for the Standard Test Tube Protocol with 3 unknowns and 2 replicates of each sample:


$$(9 \text{ standards} + 3 \text{ unknowns}) \times (2 \text{ replicates}) \times (2 \text{ ml}) = 48 \text{ ml WR required}$$

**Note:** 2.0 ml of the WR is required for each sample in the Test Tube Procedure, while only 200  $\mu$ l of WR reagent is required for each sample in the Microplate Procedure.

- Prepare WR by mixing 50 parts of BCA™ Reagent A with 1 part of BCA™ Reagent B (50:1, Reagent A:B). For the above example, combine 50 ml of Reagent A with 1 ml of Reagent B.

**Note:** When Reagent B is first added to Reagent A, a turbidity is observed that quickly disappears upon mixing to yield a clear, green WR. Prepare sufficient volume of WR based on the number of samples to be assayed. The WR is stable for several days when stored in a closed container at room temperature (RT).

## Procedure Summary (Test Tube Procedure, Standard Protocol)

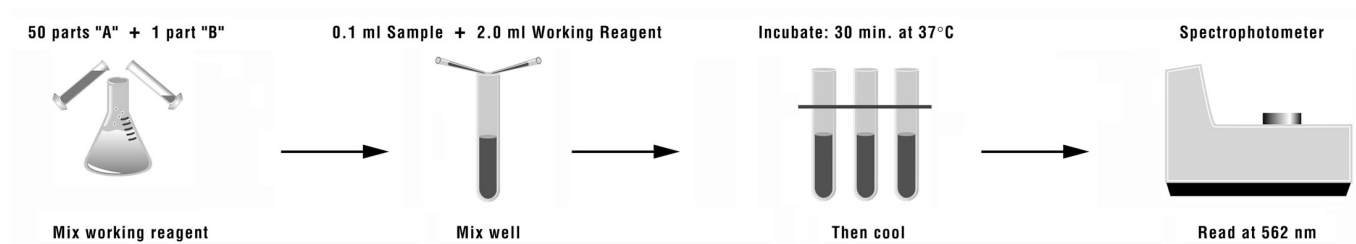

### Test Tube Procedure (Sample to WR ratio = 1:20)

1. Pipette 0.1 ml of each standard and unknown sample replicate into an appropriately labeled test tube.
2. Add 2.0 ml of the WR to each tube and mix well.
3. Cover and incubate tubes at selected temperature and time:

Standard Protocol: 37°C for 30 minutes (working range = 20-2,000 µg/ml)

RT Protocol: RT for 2 hours (working range = 20-2,000 µg/ml)

Enhanced Protocol: 60°C for 30 minutes (working range = 5-250 µg/ml)

#### Notes:

Increasing the incubation time or temperature increases the net 562 nm absorbance for each test and decreases both the minimum detection level of the reagent and the working range of the protocol.

Use a water bath to heat tubes for either Standard (37°C incubation) or Enhanced (60°C incubation) Protocol. Using a forced-air incubator can introduce significant error in color development because of uneven heat transfer.

4. Cool all tubes to RT.
5. With the spectrophotometer set to 562 nm, zero the instrument on a cuvette filled only with water. Subsequently, measure the absorbance of all the samples within 10 minutes.

**Note:** Because the BCA™ Assay does not reach a true end point, color development will continue even after cooling to RT. However, because the rate of color development is low at RT, no significant error will be introduced if the 562 nm absorbance measurements of all tubes are made within 10 minutes of each other.

6. Subtract the average 562 nm absorbance measurement of the Blank standard replicates from the 562 nm absorbance measurement of all other individual standard and unknown sample replicates.
7. Prepare a standard curve by plotting the average Blank-corrected 562 nm measurement for each BSA standard vs. its concentration in µg/ml. Use the standard curve to determine the protein concentration of each unknown sample.

### Microplate Procedure (Sample to WR ratio = 1:8)

1. Pipette 25 µl of each standard or unknown sample replicate into a microplate well (working range = 20-2,000 µg/ml).

**Note:** If sample size is limited, 10 µl of each unknown sample and standard can be used (sample to WR ratio = 1:20). However, the working range of the assay in this case will be limited to 125-2,000 µg/ml.

2. Add 200 µl of the WR to each well and mix plate thoroughly on a plate shaker for 30 seconds.
3. Cover plate and incubate at 37°C for 30 minutes.
4. Cool plate to RT.
5. Measure the absorbance at or near 562 nm on a plate reader.

#### Notes:

Wavelengths from 540-590 nm have been used successfully with this method.

Because plate readers use a shorter light path length than cuvette spectrophotometers, the Microplate Procedure requires a greater sample to WR ratio to obtain the same sensitivity as the standard Test Tube Procedure. If higher 562 nm measurements are desired, increase the incubation time to 2 hours.

Increasing the incubation time or ratio of sample volume to WR increases the net 562 nm measurement for each well and lowers both the minimum detection level of the reagent and the working range of the assay. As long as all standards and unknowns are treated identically, such modifications may be useful.

6. Subtract the average 562 nm absorbance measurement of the Blank standard replicates from the 562 nm measurements of all other individual standard and unknown sample replicates.
7. Prepare a standard curve by plotting the average Blank-corrected 562 nm measurement for each BSA standard vs. its concentration in  $\mu\text{g/ml}$ . Use the standard curve to determine the protein concentration of each unknown sample.

**Note:** If using curve-fitting algorithms associated with a microplate reader, a four-parameter (quadratic) or best-fit curve will provide more accurate results than a purely linear fit. If plotting results by hand, a point-to-point curve is preferable to a linear fit to the standard points.

## Troubleshooting

Problem	Possible Cause	Solution
No color in any tubes	Sample contains a copper chelating agent	Dialyze, desalt, or dilute sample Increase copper concentration in working reagent (e.g., use 50:2, Reagent A:B) Remove interfering substances from sample using Product No. 23215
Blank absorbance is OK, but standards and samples show less color than expected	Strong acid or alkaline buffer, alters working reagent pH	Dialyze, desalt, or dilute sample
	Color measured at the wrong wavelength	Measure the absorbance at 562 nm
Color of samples appears darker than expected	Protein concentration is too high	Dilute sample
	Sample contains lipids or lipoproteins	Add 2% SDS to the sample to eliminate interference from lipids <sup>3</sup> Remove interfering substances from sample using Product No. 23215
All tubes (including blank) are dark purple	Buffer contains a reducing agent	Dialyze or dilute sample Remove interfering substances from sample using Product No. 23215
	Buffer contains a thiol	
	Buffer contains biogenic amines (catecholamines)	
Need to measure color at a different wavelength	Spectrophotometer or plate reader does not have 562 nm filter	Color may be measure at any wavelength between 540 nm and 590 nm, although the slope of standard curve and overall assay sensitivity will be reduced

### A. Interfering substances

Certain substances are known to interfere with the BCA™ Assay including those with reducing potential, chelating agents, and strong acids or bases. Because they are known to interfere with protein estimation at even minute concentrations, avoid the following substances as components of the sample buffer:

Ascorbic Acid	EGTA	Iron	Impure Sucrose
Catecholamines	Impure Glycerol	Lipids	Tryptophan
Creatinine	Hydrogen Peroxide	Melibiose	Tyrosine
Cysteine	Hydrazides	Phenol Red	Uric Acid

Other substances interfere to a lesser extent with protein estimation using the BCA™ Assay, and these have only minor (tolerable) effects below a certain concentration in the original sample. Maximum compatible concentrations for many substances in the Standard Test Tube Protocol are listed in Table 2 (see last page of Instructions). Substances were compatible at the indicated concentration in the Standard Test Tube Protocol if the error in protein concentration estimation caused by the presence of the substance in the sample was less than or equal to 10%. The substances were tested using WR prepared immediately before each experiment. Blank-corrected 562 nm absorbance measurements (for a 1,000  $\mu\text{g/ml}$  BSA standard + substance) were compared to the net 562 nm measurements of the same standard prepared in 0.9% saline. In the Microplate Procedure, where the sample to WR ratio is 1:8 (v/v), maximum compatible concentrations will be lower.

**B. Strategies for eliminating or minimizing the effects of interfering substances**

The effects of interfering substances in the BCA™ Protein Assay may be eliminated or overcome by one of several methods.

Remove the interfering substance by dialysis or gel filtration.

Dilute the sample until the substance no longer interferes. This strategy is effective only if the starting protein concentration is sufficient to remain in the working range of the assay upon dilution.

Precipitate the proteins in the sample with acetone or trichloroacetic acid (TCA). The liquid containing the substance that interfered is discarded and the protein pellet is easily solubilized in ultrapure water or directly in the alkaline BCA™ WR.<sup>4</sup> A protocol for performing this on samples to be assayed with BCA™ Protein Assay Reagent is available at the Pierce web site. Alternatively, Product No. 23215 may be used (see Related Pierce Products).

Increase the amount of copper in the WR (prepare WR as 50:2 or 50:3, Reagent A:B), which may eliminate interference by copper chelating agents.

**Note:** For greatest accuracy, the protein standards must be treated identically to the sample(s).

**Related Pierce Products**

- 23209            **Albumin Standard Ampules, 2 mg/ml**, 10 x 1 ml ampules, containing bovine serum albumin (BSA) at 2.0 mg/ml in 0.9% saline and 0.05% sodium azide
- 23208            **Pre-Diluted Protein Assay Standards: Bovine Serum Albumin (BSA) Set**, 7 x 3.5 ml aliquots in the range of 125-2,000 g/ml
- 23212            **Bovine Gamma Globulin Standard, 2 mg/ml**, 10 x 1 ml ampules
- 23213            **Pre-Diluted Protein Assay Standards, Bovine Gamma Globulin Fraction II (BGG) Set**, 7 x 3.5 ml aliquots in the range of 125-2,000 g/ml
- 23221            **BCA™ Reagent A**, 1,000 ml
- 23223            **BCA™ Reagent A**, 250 ml
- 23224            **BCA™ Reagent B**, 25 ml
- 23235            **Micro BCA™ Protein Assay Kit**, working range of 0.5-20 g/ml
- 23236            **Coomassie Plus™ Protein Assay Kit**, working range of 1-1,500 g/ml
- 23215            **Compat-Able™ Protein Assay Preparation Reagent Set**, sufficient reagents to pre-treat 500 samples to remove interfering substances before total protein quantitation

**Additional Information**

**A. Please visit the Pierce web site for additional information on this product including the following items:**

Frequently Asked Questions


Tech Tip protocol: Eliminate interfering substances from samples for BCA™ Protein Assay

Tech Tip protocol: Shorten BCA™ Protein Assay incubation using a microwave oven

**B. Response characteristics for different proteins**

Each of the commonly used total protein assay methods exhibits some degree of varying response toward different proteins. These differences relate to amino acid sequence, pI, structure and the presence of certain side chains or prosthetic groups that can dramatically alter the protein's color response. Most protein assay methods utilize BSA or immunoglobulin (IgG) as the standard against which the concentration of protein in the sample is determined (Figure 1). However, if great accuracy is required, the standard curve should be prepared from a pure sample of the target protein to be measured.

Table 3 shows typical BCA™ Protein Assay protein-to-protein variation in color response. All proteins were tested at a concentration of 1,000 µg/ml using the 30-minute/37°C Test Tube Protocol. The average net color response for BSA was normalized to 1.00 and the average net color response of the other proteins is expressed as a ratio to the response of BSA.

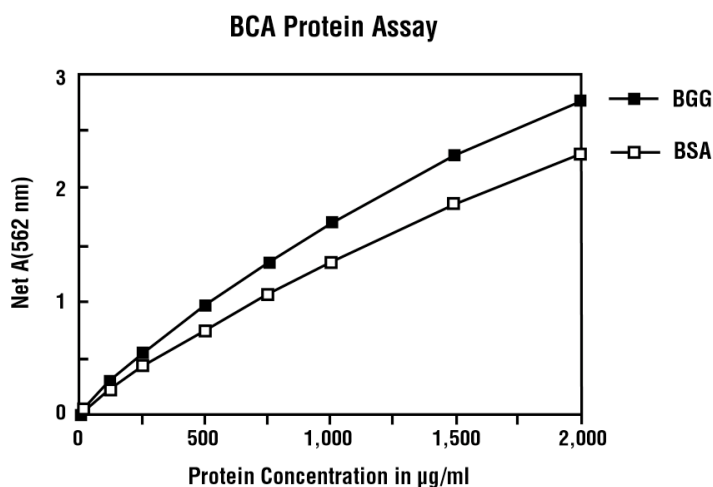

**Figure 1:** Typical color response curves for BSA and BGG using the Standard Test Tube Protocol (37°C/30-minute incubation).

**Table 3.** Protein-to-Protein Variation. Absorbance ratios (562 nm) for proteins relative to BSA using the Standard Test Tube Protocol.

Ratio = (Avg "test" net Abs.) / (avg. BSA net Abs.)	
<u>Protein Tested</u>	<u>Ratio</u>
Albumin, bovine serum	1.00
Aldolase, rabbit muscle	0.85
α-Chymotrypsinogen, bovine	1.14
Cytochrome C, horse heart	0.83
Gamma globulin, bovine	1.11
IgG, bovine	1.21
IgG, human	1.09
IgG, mouse	1.18
IgG, rabbit	1.12
IgG, sheep	1.17
Insulin, bovine pancreas	1.08
Myoglobin, horse heart	0.74
Ovalbumin	0.93
Transferrin, human	0.89
<b>Average ratio</b>	<b>1.02</b>
<b>Standard Deviation</b>	<b>0.15</b>
<b>Coefficient of Variation</b>	<b>14.7%</b>

**C. Alternative Total Protein Assay Reagents**

If interference by a reducing substance or metal-chelating substance contained in the sample cannot be overcome, try the Coomassie Plus™ Protein Assay Kit (Product No. 23236), which is less sensitive to such substances.

**D. Cleaning and Re-using Glassware**

Exercise care when re-using glassware. All glassware must be cleaned and given a thorough final rinse with ultrapure water.

**Cited References**

1. Smith, P.K., *et al.* (1985). Measurement of protein using bicinchoninic acid. *Anal. Biochem.* **150**:76-85.
2. Wiechelmann, K., Braun, R. and Fitzpatrick, J. (1988). Investigation of the bicinchoninic acid protein assay: Identification of the groups responsible for color formation. *Anal Biochem.* **175**:231-7.
3. Kessler, R. and Fanestil, D. (1986). Interference by lipids in the determination of protein using bicinchoninic acid. *Anal. Biochem.* **159**:138-42.
4. Brown, R., Jarvis, K. and Hyland, K. (1989). Protein measurement using bicinchoninic acid: elimination of interfering substances. *Anal. Biochem.* **180**:136-9.

**Product References**

- Adilakshami, T. and Laine, R.O. (2002). Ribosomal protein S25 mRNA partners with MTF-1 and La to provide a p53-mediated mechanism for survival or death. *J. Biol. Chem.* **277**:4147-51.
- Fischer, T., *et al.* (1999). Clathrin-coated vesicles bearing GAIP possess GTPase-activating protein activity in vitro. *Proc. Nat. Acad. Sci.* **96**:6722-7.
- Prozialeck, W.C., *et al.* (2002). Chlamydia trachomatis disrupts N-cadherin-dependent cell-cell junctions and sequester β-catenin in human cervical epithelial cells. *Infection and Immunity* **70**:2605-13.
- Roberts, K.P., Ensrud, K.M. and Hamilton, D.W. (2002). A comparative analysis of expression and processing of the rat epididymal fluid and sperm-bound forms of proteins D and E. *Biology of Reproduction* **67**:525-33.

Triton® is a registered trademark of Rohm & Haas Co.  
 Brij® , Tween® and Span® are registered trademarks of ICI Americas.  
 Zwittergent® is a registered trademark of American Hoechst Corporation.  
 The BCA™ Protein Assay is protected by U.S. Patent # 4,839,295

©Pierce Biotechnology, Inc., 10/2003. Printed in the USA.



**Table 2.** Compatible Substance Concentrations in the BCA™ Protein Assay (see text for details).

Substance	Compatible Concentration	Substance	Compatible Concentration
<b>Salts/Buffers</b>		<b>Detergents**</b>	
ACES, pH 7.8	25 mM	Brij®-35	5.0%
Ammonium sulfate	1.5 M	Brij®-56, Brij®-58	1.0%
Asparagine	1 mM	CHAPS, CHAPSO	5.0%
Bicine, pH 8.4	20 mM	Deoxycholic acid	5.0%
Bis-Tris, pH 6.5	33 mM	Octyl β-glucoside	5.0%
Borate (50 mM), pH 8.5 (#28384)	undiluted	Nonidet P-40 (NP-40)	5.0%
B-PER® Reagent (#78248)	undiluted	Octyl β-thioglucoopyranoside	5.0%
Calcium chloride in TBS, pH 7.2	10 mM	SDS	5.0%
Na-Carbonate/Na-Bicarbonate (0.2 M), pH 9.4 (#28382)	undiluted	Span® 20	1.0%
Cesium bicarbonate	100 mM	Triton® X-100	5.0%
CHES, pH 9.0	100 mM	Triton® X-114, X-305, X-405	1.0%
Na-Citrate (0.6 M), Na-Carbonate (0.1 M), pH 9.0 (#28388)	1:8 dilution*	Tween®-20, Tween®-60, Tween®-80	5.0%
Na-Citrate (0.6 M), MOPS (0.1 M), pH 7.5 (#28386)	1:8 dilution*	Zwittergent® 3-14	1.0%
Cobalt chloride in TBS, pH 7.2	0.8 mM	<b>Chelating agents</b>	
EPPS, pH 8.0	100 mM	EDTA	10 mM
Ferric chloride in TBS, pH 7.2	10 mM	EGTA	-----
Glycine•HCl, pH 2.8	100 mM	Sodium citrate	200 mM
Guanidine•HCl	4 M	<b>Reducing &amp; Thiol-Containing Agents</b>	
HEPES, pH 7.5	100 mM	<i>N</i> -acetylglucosamine in PBS, pH 7.2	10 mM
Imidazole, pH 7.0	50 mM	Ascorbic acid	-----
MES, pH 6.1	100 mM	Cysteine	-----
MES (0.1 M), NaCl (0.9%), pH 4.7 (#28390)	undiluted	Dithioerythritol (DTE)	1 mM
MOPS, pH 7.2	100 mM	Dithiothreitol (DTT)	1 mM
Modified Dulbecco's PBS, pH 7.4 (#28374)	undiluted	Glucose	10 mM
Nickel chloride in TBS, pH 7.2	10 mM	Melibiose	-----
PBS; Phosphate (0.1 M), NaCl (0.15 M), pH 7.2 (#28372)	undiluted	2-Mercaptoethanol	0.01%
PIPES, pH 6.8	100 mM	Potassium thiocyanate	3.0 M
RIPA lysis buffer; 50 mM Tris, 150 mM NaCl, 0.5% DOC, 1% NP-40, 0.1% SDS, pH 8.0	undiluted	Thimerosal	0.01%
Sodium acetate, pH 4.8	200 mM	<b>Misc. Reagents &amp; Solvents</b>	
Sodium azide	0.2%	Acetone	10%
Sodium bicarbonate	100 mM	Acetonitrile	10%
Sodium chloride	1 M	Aprotinin	10 mg/L
Sodium citrate, pH 4.8 or pH 6.4	200 mM	DMF, DMSO	10%
Sodium phosphate	100 mM	DMSO	10%
Tricine, pH 8.0	25 mM	Ethanol	10%
Triethanolamine, pH 7.8	25 mM	Glycerol (Fresh)	10%
Tris	250 mM	Hydrazides	-----
TBS; Tris (25 mM), NaCl (0.15 M), pH 7.6 (#28376)	undiluted	Hydrides (Na <sub>2</sub> BH <sub>4</sub> or NaCNBH <sub>3</sub> )	-----
Tris (25 mM), Glycine (192 mM), pH 8.0 (#28380)	1:3 dilution*	Hydrochloric Acid	100 mM
Tris (25 mM), Glycine (192 mM), SDS (0.1%), pH 8.3 (#28378)	undiluted	Leupeptin	10 mg/L
Zinc chloride in TBS, pH 7.2	10 mM	Methanol	10%
		Phenol Red	-----
		PMSF	1 mM
		Sodium Hydroxide	100 mM
		Sucrose	40%
		TLCK	0.1 mg/L
		TPCK	0.1 mg/L
		Urea	3 M
		o-Vanadate (sodium salt), in PBS, pH 7.2	1 mM

\* Diluted with ultrapure water; \*\* Detergents were tested using Pierce high-purity Surfact-Amps™ Products, which have low peroxide content; -- Dashed-line entry indicates that the material is incompatible with the assay.